

PEXLITH

CERTIFICATE OF ANALYSIS

Reconstitution Solution (10mL)

BATCH / LOT

26VBAS124

TESTING DATE

2026-07-16

TESTING LABORATORY

Accumark Labs


Pexlith company branding. Laboratory test data, signatures and verification information retained.



Pexlith

SAMPLE NAME:
SAMPLE CODE:
RECEIVED DATE:
PUBLISHED DATE:

Reconstitution Solution
FAUP-TTQX
07/13/2026
07/16/2026

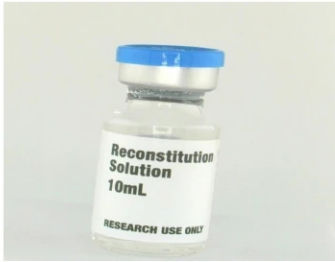

DECLARED IDENTITY

Bacteriostatic Water

MATRIX TYPE:

BACTERIOSTATIC WATER

SAMPLE NAME:

Reconstitution Solution

SAMPLE SIZE:


10 mL

LOT CODE:

26VBAS124

Sample	Test	Specification	Result	Status
Benzyl Alcohol Assay (HPLC)	HPLC	0.9% (v/v) $\pm$ 10%	0.88 % (v/v)	CONFORMS
Fill volume / Net content	Gravimetric	—	10.24 mL	MEASURED
pH Determination	pH	4.5 – 7.0	6.71	CONFORMS

HPLC Chromatogram Report

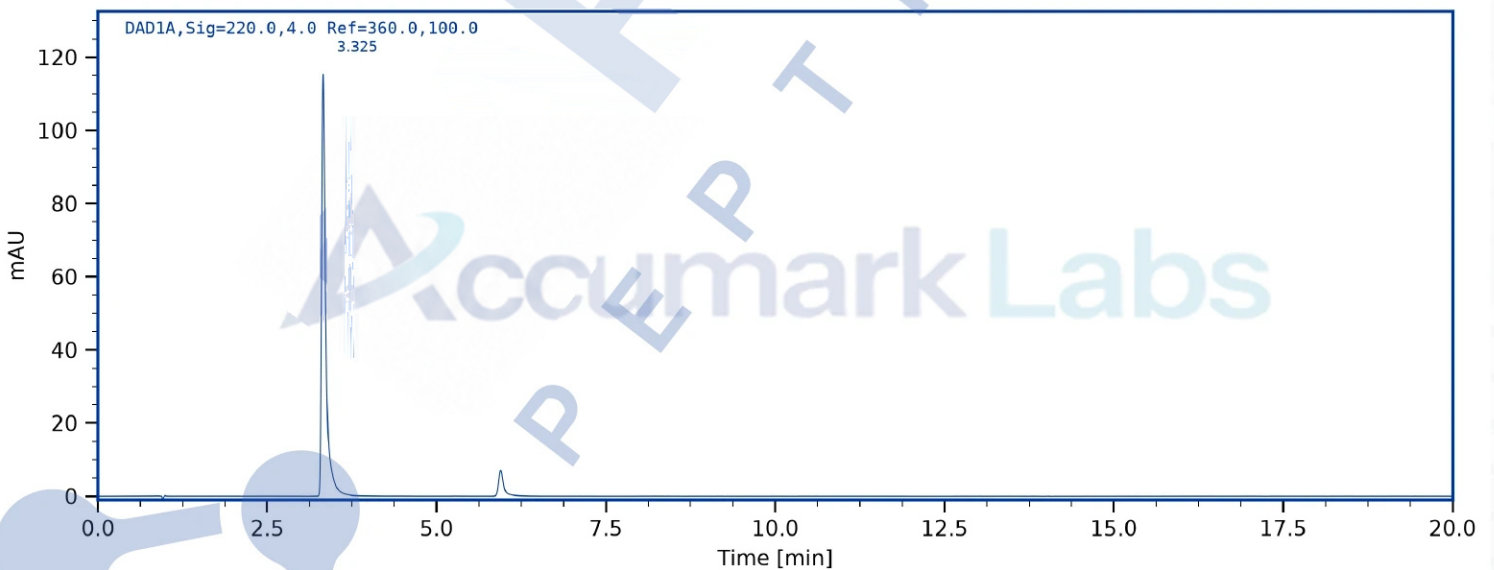

RESULTS REVIEWED BY:

Anthony Burke PhD
Lab Manager
07/16/2026

RESULTS CERTIFIED BY:

Dr. Levi Fried MD
Lab Director
07/16/2026

ACCUMARKLABS.COM
FAUP-TTQX
07/16/2026





Pexlith

SAMPLE NAME:
SAMPLE CODE:
RECEIVED DATE:
PUBLISHED DATE:

Reconstitution Solution
FAUP-TTQX
07/13/2026
07/16/2026

Sample	Test	Specification	Result	Status
Reconstitution Solution	Endotoxin (LAL)	≤ 0.25 EU/mL	Pass	CONFORMS
Reconstitution Solution	Rapid Sterility Screening (PCR)	Not Detected	Pass	CONFORMS

PEPTIDES

RESULTS CERTIFIED BY:

RESULTS CERTIFIED BY:

Anthony Burke PhD
Lab Manager
07/16/2026

Dr. Levi Fried MD
Lab Director
07/16/2026

ACCUMARKLABS.COM
FAUP-TTQX
07/16/2026

