

PEXLITH

CERTIFICATE OF ANALYSIS

MT-II (Melanotan II) (10mg)

BATCH / LOT

MEL209032025-J

TESTING DATE

2026-07-06

TESTING LABORATORY

Accumark Labs

Pexlith company branding. Laboratory test data, signatures and verification information retained.



Pexlith

SAMPLE NAME: **Tesamorelin Melanotan II**
 SAMPLE CODE: **KU8R-8Y5G**
 RECEIVED DATE: **06/30/2026**
 PUBLISHED DATE: **07/06/2026**



DECLARED IDENTITY

Melanotan II



MATRIX TYPE:

PEPTIDE

SAMPLE NAME:

Melanotan II



10.51 mg
Total Quantity

SAMPLE SIZE:

10.0 mg

LOT CODE:


MEL209032025-J



99.72%
Total Blend Purity

Sample	Test	Specification	Result	Status
Melanotan II	IDENTITY	Melanotan II	Melanotan II	CONFORMS
Melanotan II	QUANTITY	MEASURE	10.51 mg	MEASURED
Melanotan II	PURITY	> 98.0%	99.72%	CONFORMS

HPLC Chromatogram Report

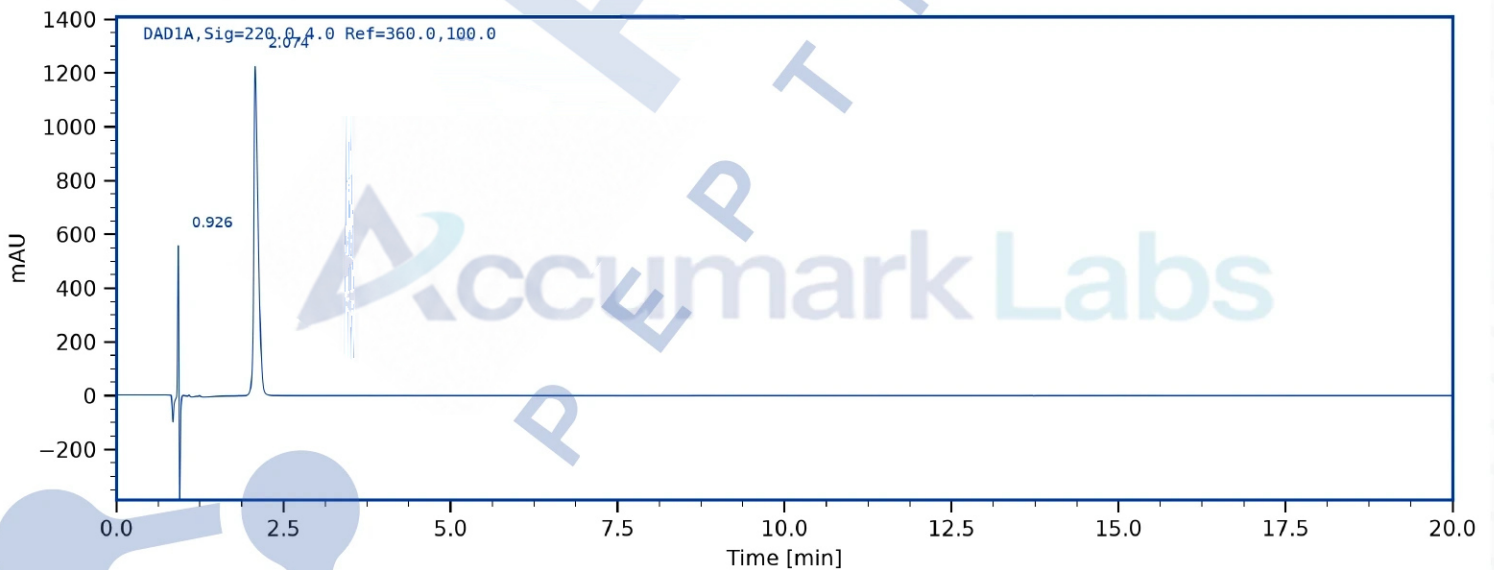

RESULTS REVIEWED BY:

Anthony Burke PhD
Lab Manager
07/06/2026

RESULTS CERTIFIED BY:

Dr. Levi Fried MD
Lab Director
07/06/2026

ACCUMARKLABS.COM
KU8R-8Y5G
07/06/2026





Pexlith

SAMPLE NAME:
SAMPLE CODE:
RECEIVED DATE:
PUBLISHED DATE:

Tesamotin Melanotan II
KU8R-8Y5G
06/30/2026
07/06/2026

Sample	Test	Specification	Result	Status
Melanotan II	Endotoxin (LAL)	≤ 5.0 EU/mL	Pass	CONFORMS
Melanotan II	Rapid Sterility Screening (PCR)	Not Detected	Pass	CONFORMS

PEPTIDES

RESULTS CERTIFIED BY:

RESULTS CERTIFIED BY:

Anthony Burke PhD
Lab Manager
07/06/2026

Dr. Levi Fried MD
Lab Director
07/06/2026

ACCUMARKLABS.COM
KU8R-8Y5G
07/06/2026

