

PEXLITH

CERTIFICATE OF ANALYSIS

Reconstitution Solution (30mL)

BATCH / LOT

26VBAS072

TESTING DATE

2026-08-07

TESTING LABORATORY

Accumark Labs

Pexlith company branding. Laboratory test data, signatures and verification information retained.



Pexlith


SAMPLE NAME: Reconstitution Solution
 SAMPLE CODE: 9HM4-PL6U
 RECEIVED DATE: 06/23/2026
 PUBLISHED DATE: 08/07/2026



DECLARED IDENTITY	Bacteriostatic Water
MATRIX TYPE:	BACTERIOSTATIC WATER
SAMPLE NAME:	Reconstitution Solution
SAMPLE SIZE:	30 mL
LOT CODE:	26VBAS072

Sample	Test	Specification	Result	Status
Benzyl Alcohol Assay (HPLC)	HPLC	0.9% (v/v) $\pm$ 20%	0.88 % (v/v)	CONFORMS
Fill volume / Net content	Gravimetric	—	30.49 mL	MEASURED
pH Determination	pH	4.5 – 7.0	6.55	CONFORMS

HPLC Chromatogram Report

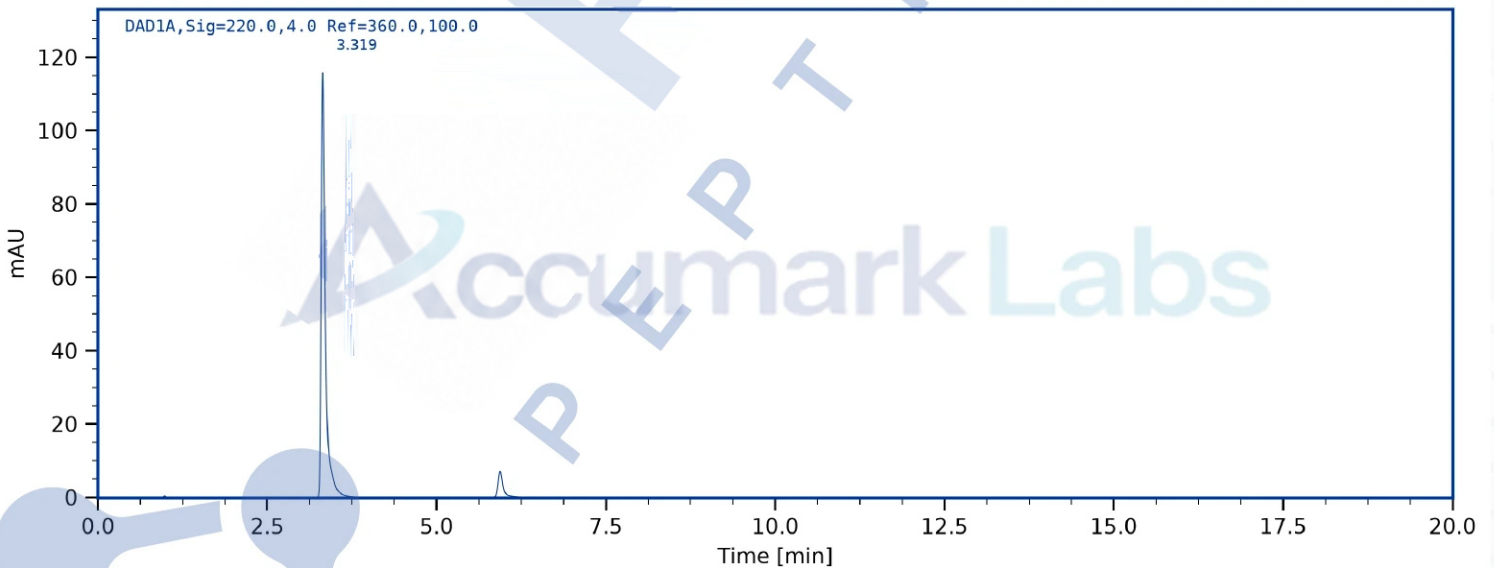

RESULTS REVIEWED BY:

Anthony Burke PhD
 Lab Manager
 08/07/2026

RESULTS CERTIFIED BY:

Dr. Levi Fried MD
 Lab Director
 08/07/2026

ACCUMARKLABS.COM
 9HM4-PL6U
 08/07/2026





Pexlith

SAMPLE NAME:
SAMPLE CODE:
RECEIVED DATE:
PUBLISHED DATE:

Reconstitution Solution
9HM4-PL6U
06/23/2026
08/07/2026

Sample	Test	Specification	Result	Status
Reconstitution Solution	Endotoxin (LAL)	≤ 0.25 EU/mL	Pass	CONFORMS
Reconstitution Solution	Rapid Sterility Screening (PCR)	Not Detected	Pass	CONFORMS

PEPTIDES

RESULTS CERTIFIED BY:

RESULTS CERTIFIED BY:

Anthony Burke
Anthony Burke PhD
Lab Manager
08/07/2026

Levi Fried
Dr. Levi Fried MD
Lab Director
08/07/2026

ACCUMARKLABS.COM
9HM4-PL6U
08/07/2026

